



Cancel

MAUI


2026/06/10 13:12 | CN 6.2.1 (GAR6) | mini 6



Support



Save

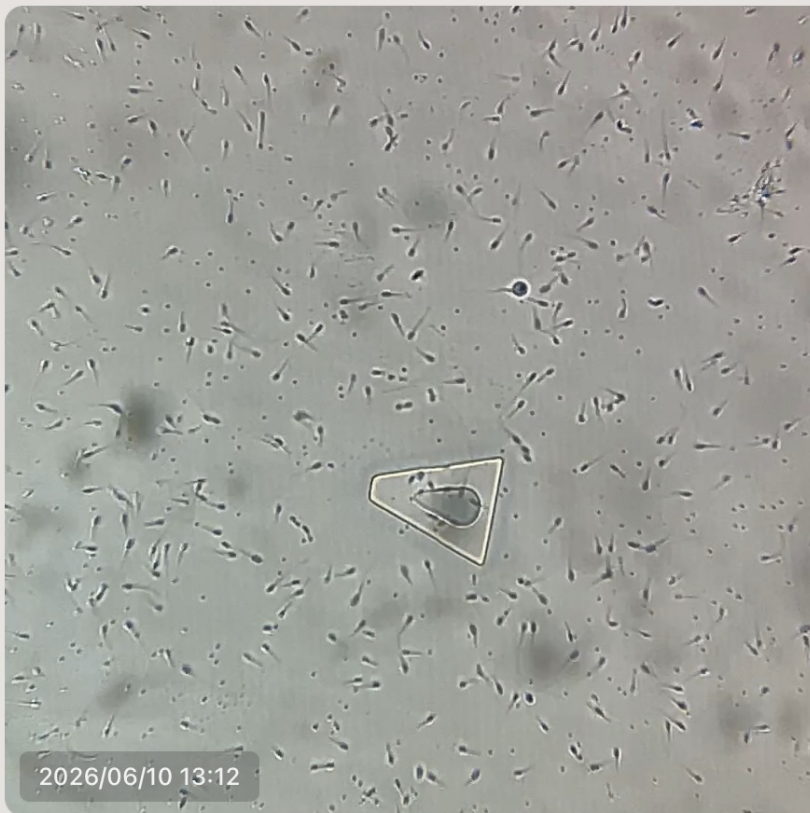

2026/06/10 13:12

Conc.	46.57 M/ml
Motile	97 %
Progressive	91 %
VCL	196 $\mu\text{m/s}$
VAP	112 $\mu\text{m/s}$
VSL	99 $\mu\text{m/s}$
STR	87 %
LIN	51 %
BCF	24 Hz
ALH	11 μm
WOB	58 %

Draw Sperm Tracks

Fullscreen Video

Delete Record

2026/

Average of Analysis Data (4)

Show Settings

Concentration

47.13 M / ml

Motility

95 %

Progressive

86 %

Abnormality

0 %

Sperm Kinetics

VCL

192 $\mu\text{m/s}$

VAP

104 $\mu\text{m/s}$

VSL

91 $\mu\text{m/s}$

STR

85 %

LIN

47 %

BCF

24 Hz

ALH

11 μm

WOB

55 %

Information

Name

MAUI

Source

Eval

Analysis Result

Semen Extending